OpClear®

Quick Guide

BEFORE

1. Plug in Unit and Turn Main Power On
2. Attach CO2 Supply
3. Plug In Footswitch
4. Push Power Button on Front of Display
5. Toggle Between Pediatric and Adult Mode using Up/Down Arrows. Confirm Choice by Pressing Left or Right Arrow
6. Select Appropriate Size of Disposable Sheath Kit
7. Fill Saline Cartridge with 10cc of Saline
8. Wipe Down End of Lens
9. Attach Disposable Sheath to Scope
10. Attach CO2 and Saline Wash connectors to Front of Control Unit
11. Tap the Footswitch to Prime the Unit Before Entering Patient

DURING

1. Auto Demist will Turn on Automatically Once Entering Patient
2. Tap the Footswitch to Trigger a Wash Cycle
3. Unit Over Pressure Warning Pediatric 21mmHg - Adult 27mmHg

AFTER

1. Remove Disposable Sheath
2. Remove Tubing from Control Unit and Discard Disposable Kit
3. Turn OFF / Close CO2 Supply
4. Push and Hold Front Power Button for 3 Sec to Depressurize Control Unit
5. Turn Off Rear Power and Store

CONTINUOUSVISION

A NEW STANDARD OF CARE

www.ciphersurgical.com

OpClear® Quick Guide

CIPHER SURGICAL

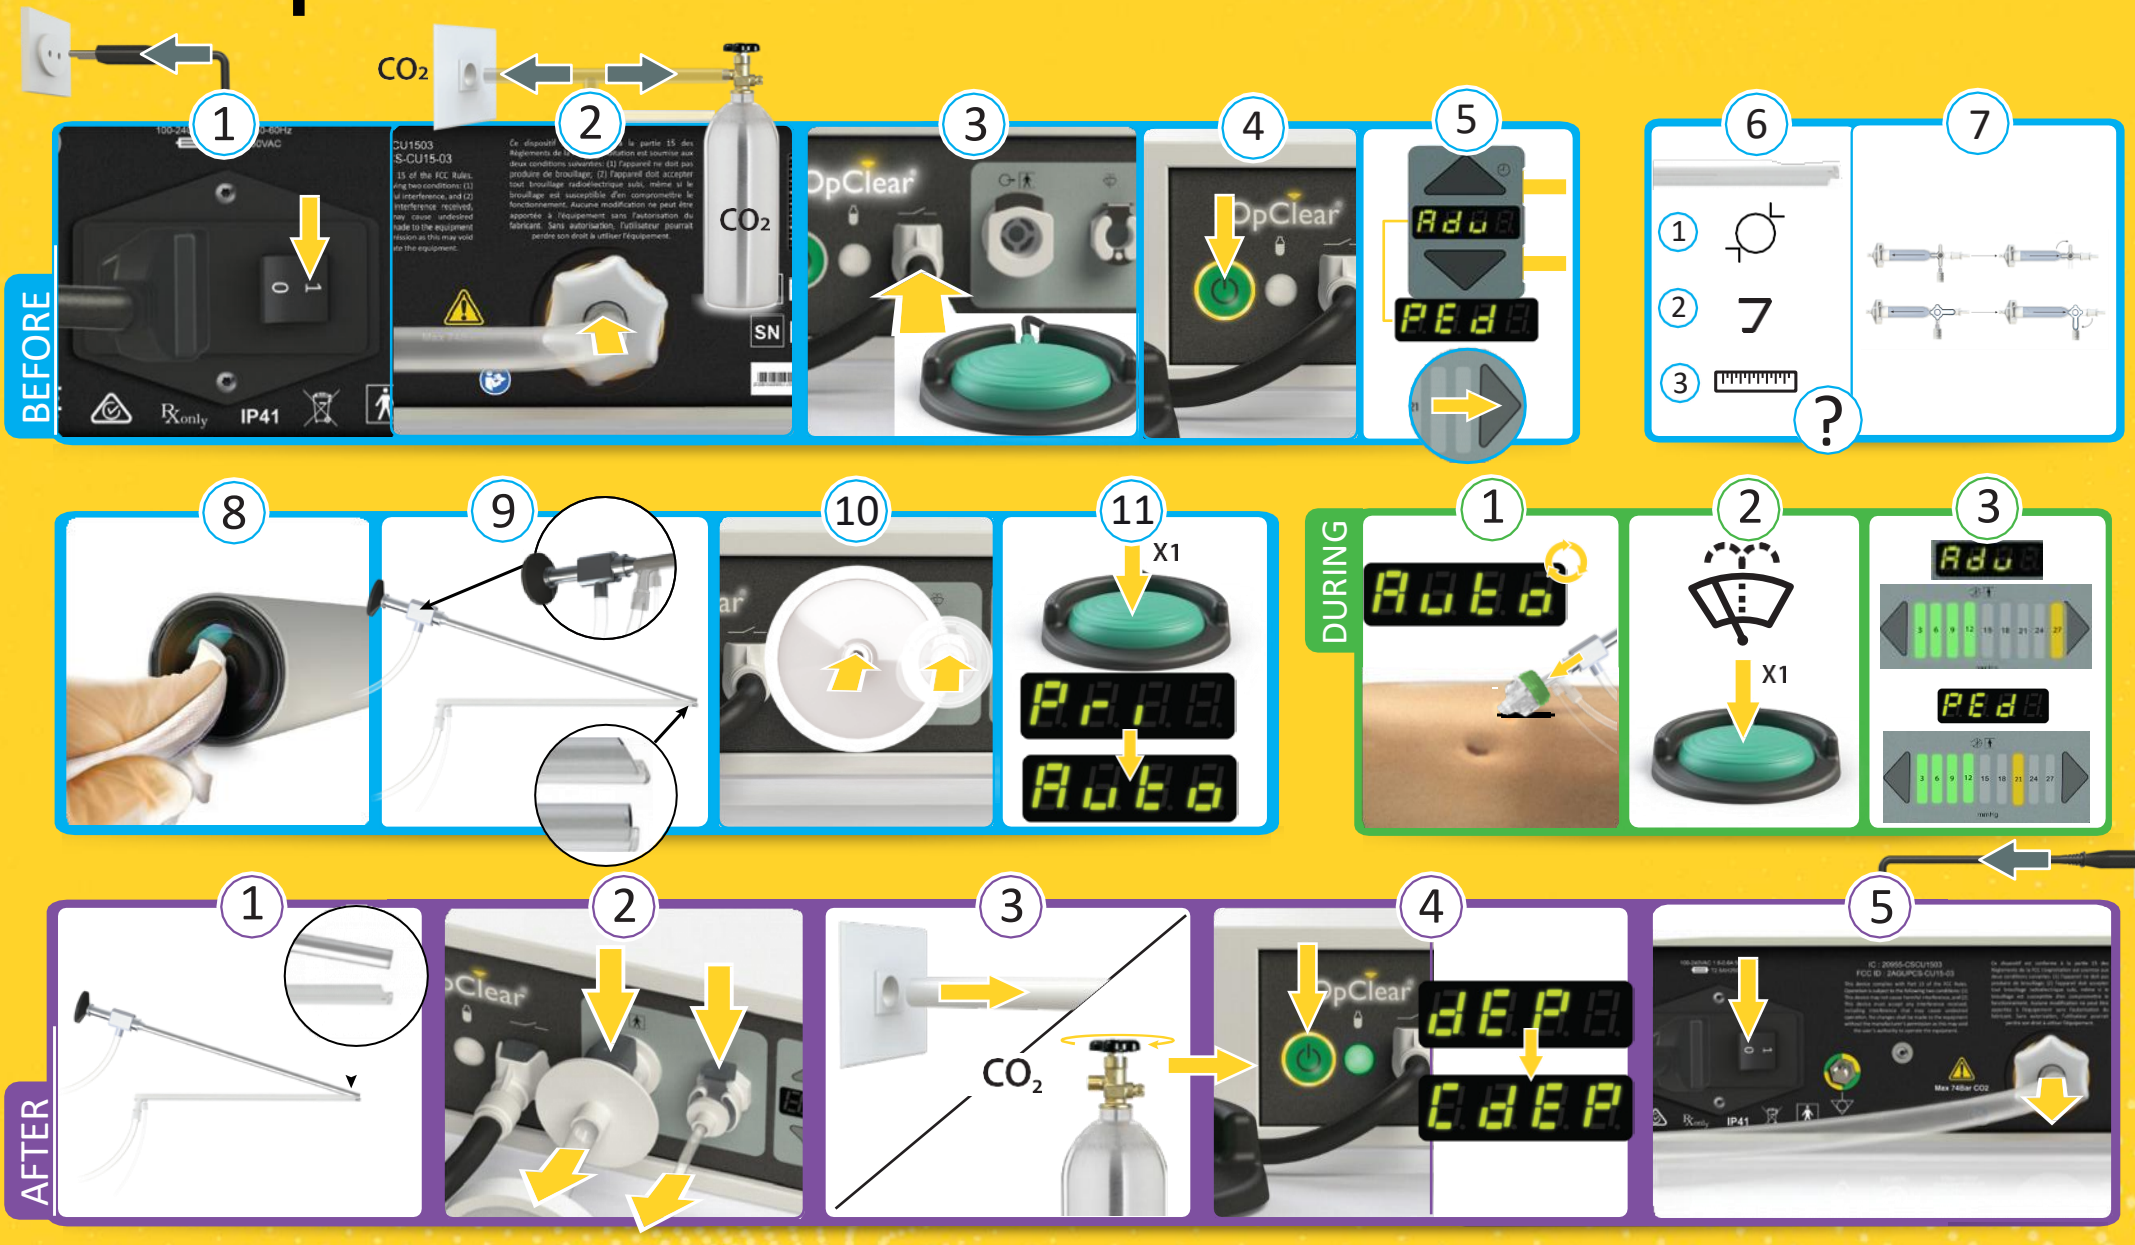

CONTINUOUSVISION

A NEW STANDARD OF CARE